


Region 6 Analytical Services Flowchart

*The Data Requestor should contact the R6SCC or review the Internet tables to determine if the Region 6 Laboratory/ESAT or CLP can perform the analysis.

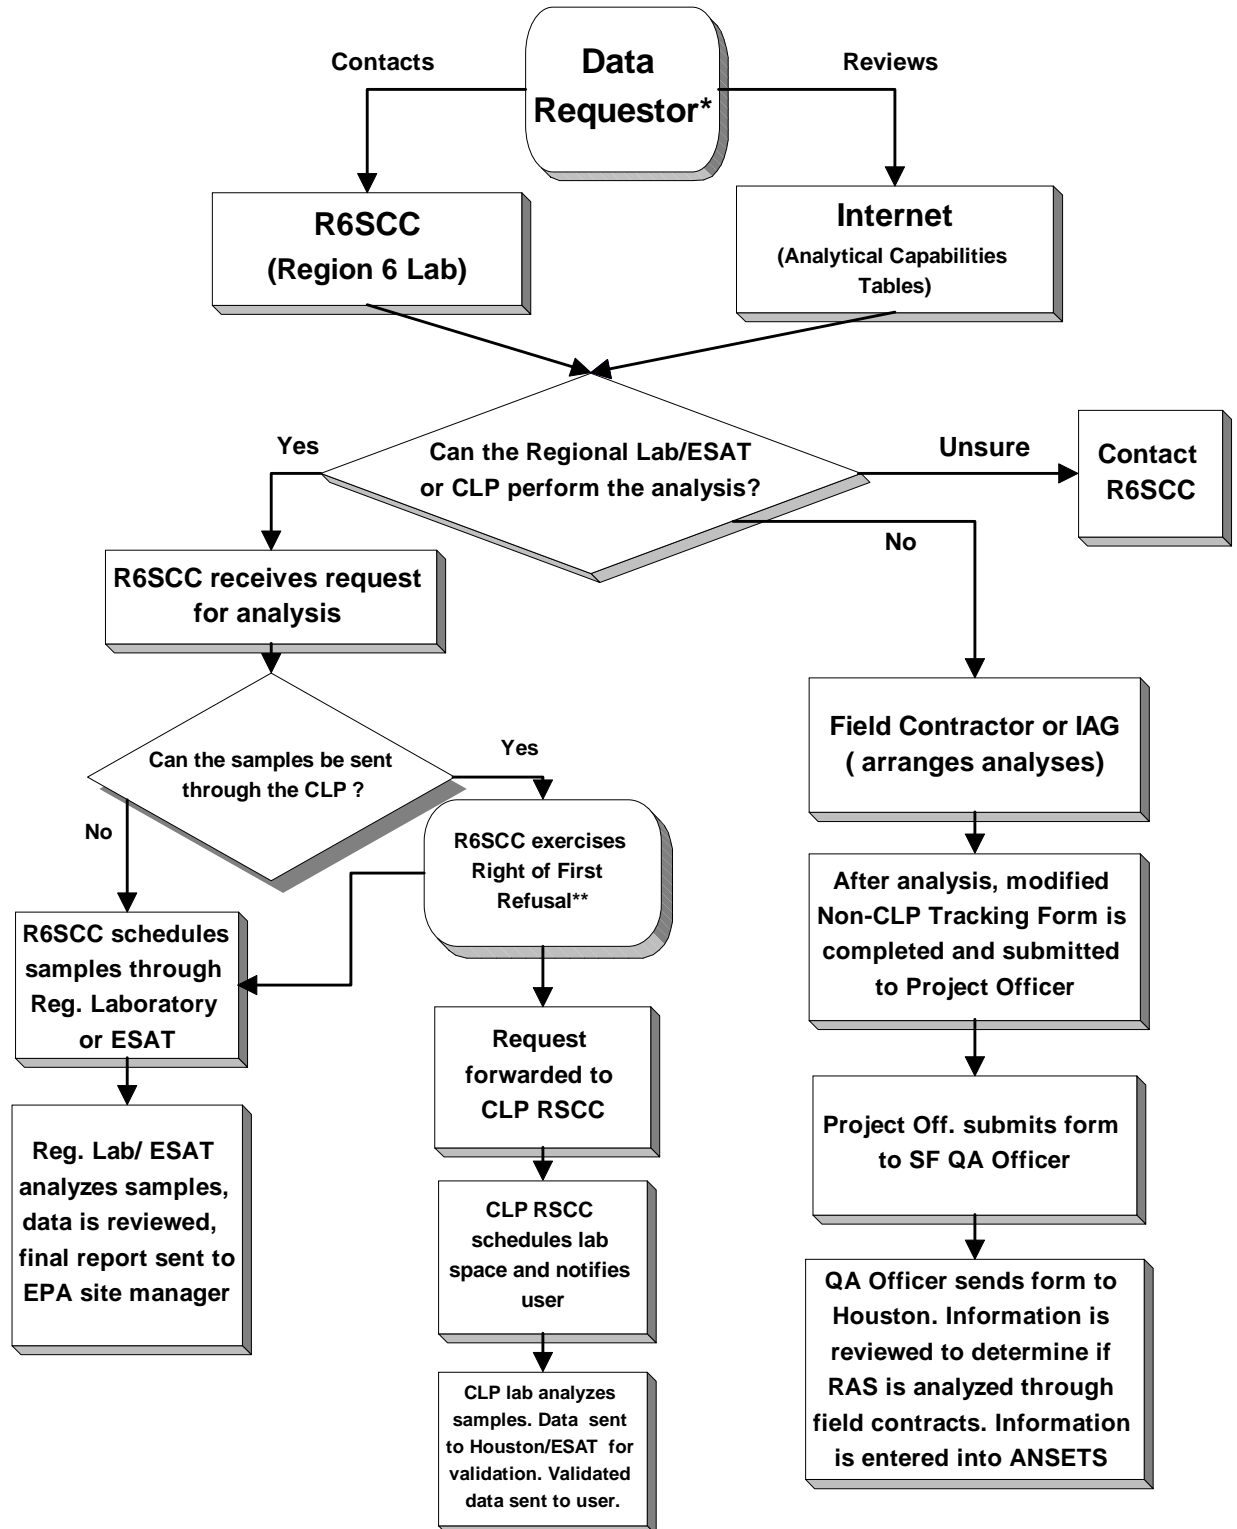

** Right of First Refusal

The Regional laboratory may choose to process RAS samples due to the following :

- 1) laboratory workload below capacity, 2) samples are from a drinking water source , 3) user preference